

GITR (DM80) RABBIT MAB

货号: 28401

产品全名: GITR(DM80) 兔单克隆抗体

基因符号 AITR; GITR; TNFRSF18; CD357

描述: GITR antibody(DM80) 兔单克隆抗体

背景: This gene encodes a member of the TNF-receptor superfamily. The encoded receptor has been shown to have increased expression upon T-cell activation; and it is thought to play a key role in dominant immunological self-tolerance maintained by CD25(+)CD4(+) regulatory T cells. Knockout studies in mice also suggest the role of this receptor is in the regulation of CD3-driven T-cell activation and programmed cell death. Three alternatively spliced transcript variants of this gene encoding distinct isoforms have been reported.

经过测试的应用: ELISA; Flow Cyt

推荐稀释比: ELISA 1:5000-10000; Flow Cyt 1:100

种属反应性: Rabbit

亚型: Rabbit IgG

纯化: Purified from cell culture supernatant by affinity chromatography

种属反应性: 人 GITR

成分: Lyophilized from sterile PBS, pH 7.4. 5% - 8% trehalose is added as protectants before lyophilization.

储存和运输: Store at -20°C to -80°C for 12 months in lyophilized form. After reconstitution, if not intended for use within a month, aliquot and store at -80°C (Avoid repeated freezing and thawing).

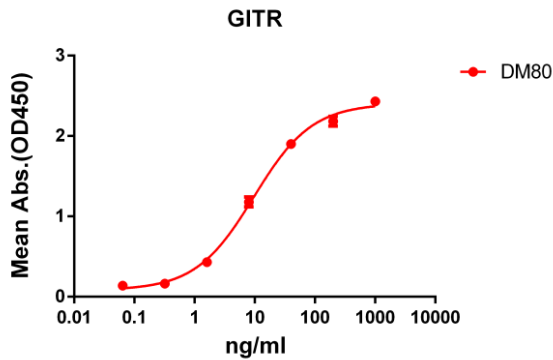


Figure 1. ELISA plate pre-coated by 2 µg/ml (100 µl/well) Human GITR protein, hFc-His tagged protein 11146 can bind Rabbit anti-GITR monoclonal antibody (clone: DM80) in a linear range of 1-100 ng/ml.

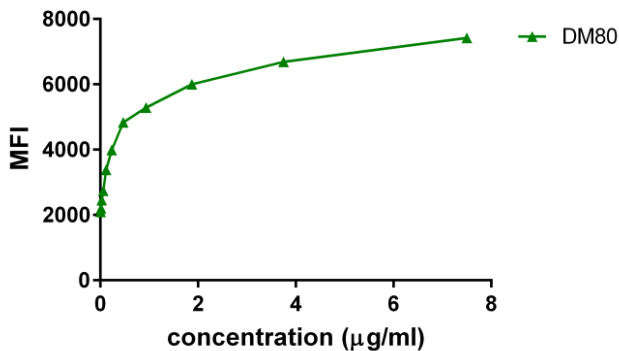


Figure 3. Flow cytometry data of serially titrated Rabbit anti-GITR monoclonal antibody (clone: DM80) on PC3 cells. The Y-axis represents the mean fluorescence intensity (MFI) while the X-axis represents the concentration of IgG used.




Figure 2. Expi 293 cell line transfected with irrelevant protein (A) and human GITR (B) were surface stained with Rabbit anti-GITR monoclonal antibody 1 µg/ml (clone: DM80) followed by Alexa 488-conjugated anti-rabbit IgG secondary antibody.

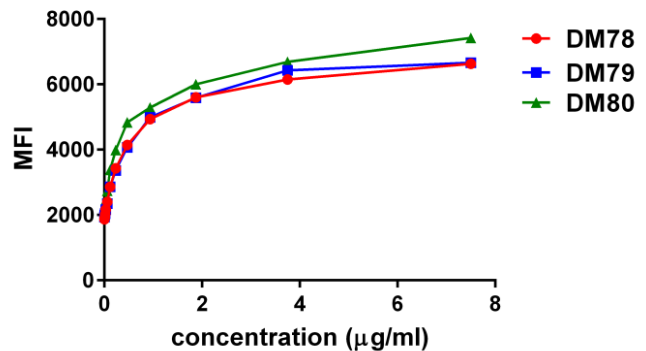


Figure 4. Affinity ranking of different Rabbit anti-GITR mAb clones by titration of different concentration onto PC3 cells. The Y-axis represents the mean fluorescence intensity (MFI) while the X-axis represents the concentration of IgG used.